


# CryoPep



Cryogenics at the service of haemostasis

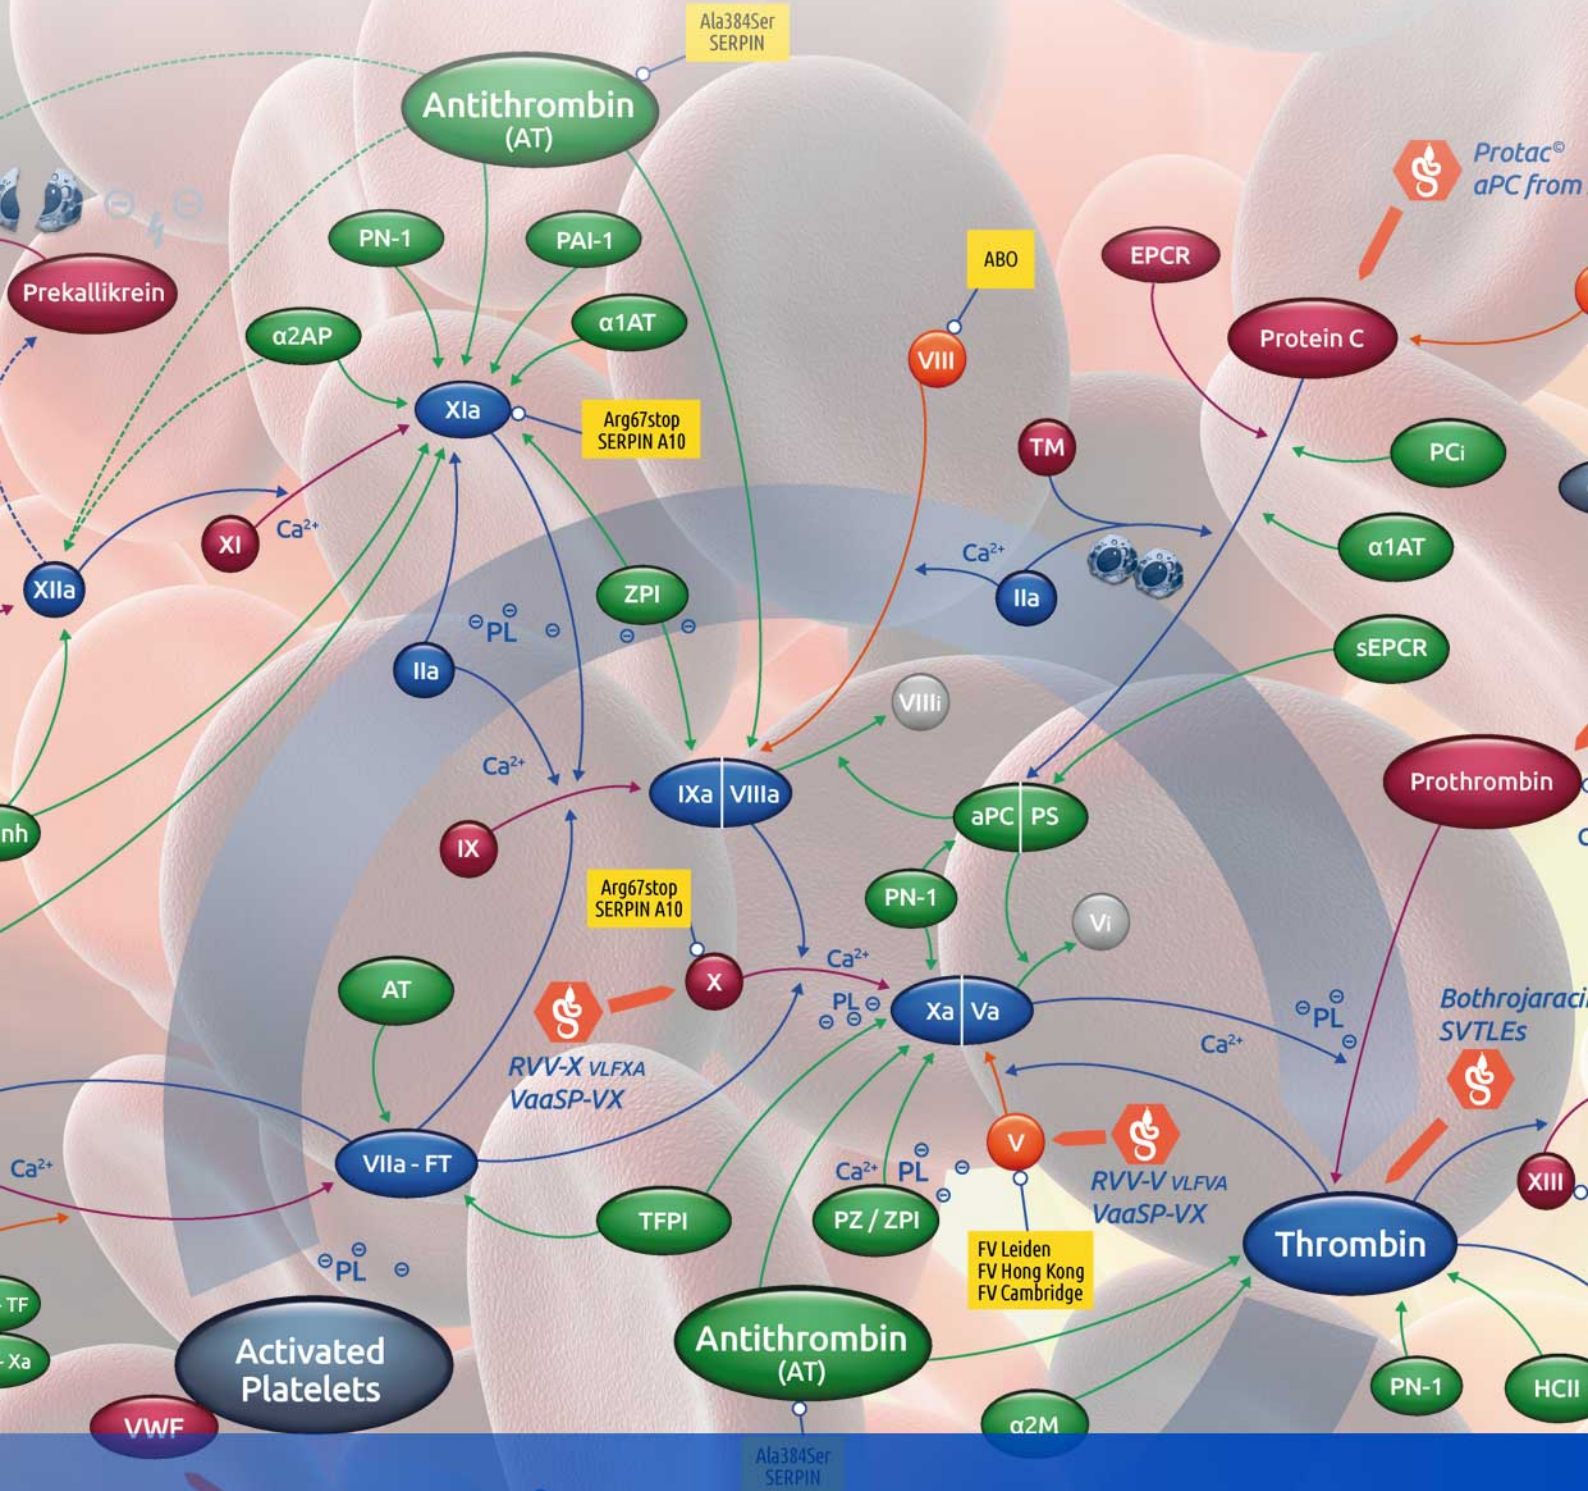

## ANTICOAGULANT MONITORING

Edition of 2024-05-03 15:05:41

way

Endothelial Cells

Bilnexin  
Convulxin  
Echicetin  
EMS16

Mucetin  
Rhodocytin  
Sochicetin-A  
Triwaglerin

# ANTICOAGULANT MONITORING

## ANTI-Xa

### ORGARAN®

#### TECHNOVIEW® Orgaran® Cal Set

| Ref       | Format     |
|-----------|------------|
| 4-5090110 | 5 x 1.0 mL |



#### TECHNOVIEW® Orgaran® Cont High

| Ref       | Format     |
|-----------|------------|
| 4-5090114 | 5 x 1.0 mL |



#### TECHNOVIEW® Orgaran® Cont Low

| Ref       | Format     |
|-----------|------------|
| 4-5090112 | 5 x 1.0 mL |



## ARIXTRA®

#### TECHNOVIEW® Arixtra® Cal Set

| Ref       | Format     |
|-----------|------------|
| 4-5090010 | 5 x 1.0 mL |



#### TECHNOVIEW® Arixtra® Cont High

| Ref       | Format     |
|-----------|------------|
| 4-5090014 | 6 x 1.0 mL |



#### TECHNOVIEW® Arixtra® Cont Low

| Ref       | Format     |
|-----------|------------|
| 4-5090012 | 6 x 1.0 mL |



## UFH

#### TECHNOVIEW® UFH Cal Set

| Ref       | Format     |
|-----------|------------|
| 4-5090070 | 5 x 1.0 mL |



#### TECHNOVIEW® UFH Cont High

| Ref       | Format     |
|-----------|------------|
| 4-5090074 | 5 x 1.0 mL |



#### TECHNOVIEW® UFH Cont Low

| Ref       | Format     |
|-----------|------------|
| 4-5090072 | 5 x 1.0 mL |



## ANTI-Xa ASSAYS

#### TECHNOCHROM® anti-Xa

| Ref       | Format    |
|-----------|-----------|
| 4-5340250 | 80 assays |



## LMW

#### TECHNOVIEW® LMW Cal Set

| Ref       | Format     |
|-----------|------------|
| 4-5090040 | 5 x 1.0 mL |



#### TECHNOVIEW® LMW Cont High

| Ref       | Format     |
|-----------|------------|
| 4-5090046 | 5 x 1.0 mL |



#### TECHNOVIEW® LMW Cont Low

| Ref       | Format     |
|-----------|------------|
| 4-5090042 | 5 x 1.0 mL |





# ANTICOAGULANT MONITORING

## TECHNOVIEW® LMW Cont Medium

| Ref       | Format     |
|-----------|------------|
| 4-5090044 | 5 x 1.0 mL |



## ANTI-IIa

### HEPARIN NEUTRALIZATION

#### HRRS Solution CaCl2 0.025M neutralizing UFH

| Ref      | Format    |
|----------|-----------|
| 20-X9107 | 5 x 10 mL |



## ANTI-IIa ASSAYS

### TECHNOCLOT® DTI

| Ref       | Format        |
|-----------|---------------|
| 4-5100025 | 2 x 20 assays |



## DOAC

### EDOXABAN

#### TECHNOVIEW® Edoxaban Cal Set

| Ref       | Format     |
|-----------|------------|
| 4-5090250 | 5 x 1.0 mL |



#### TECHNOVIEW® Edoxaban Cont High

| Ref       | Format     |
|-----------|------------|
| 4-5090253 | 5 x 1.0 mL |



#### TECHNOVIEW® Edoxaban Cont Low

| Ref       | Format     |
|-----------|------------|
| 4-5090251 | 5 x 1.0 mL |



#### TECHNOVIEW® Edoxaban Cont Medium

| Ref       | Format     |
|-----------|------------|
| 4-5090252 | 5 x 1.0 mL |



# ANTICOAGULANT MONITORING

## DABIGATRAN

### TECHNOVIEW® Dabigatran Cal Set



| Ref       | Format     |
|-----------|------------|
| 4-5090210 | 4 x 1.0 mL |



### TECHNOVIEW® Dabigatran Cont High



| Ref       | Format     |
|-----------|------------|
| 4-5090212 | 5 x 1.0 mL |



### TECHNOVIEW® Dabigatran Cont Low



| Ref       | Format     |
|-----------|------------|
| 4-5090214 | 5 x 1.0 mL |



## ARGATROBAN

### TECHNOVIEW® Argatroban Cal Set



| Ref       | Format     |
|-----------|------------|
| 4-5090140 | 5 x 1.0 mL |



### TECHNOVIEW® Argatroban Cont High



| Ref       | Format     |
|-----------|------------|
| 4-5090144 | 5 x 1.0 mL |



### TECHNOVIEW® Argatroban Cont Low



| Ref       | Format     |
|-----------|------------|
| 4-5090142 | 5 x 1.0 mL |



## RIVAROXABAN

### TECHNOVIEW® Rivaroxaban Cal Set



| Ref       | Format     |
|-----------|------------|
| 4-5090170 | 5 x 1.0 mL |



### TECHNOVIEW® Rivaroxaban Cont High



| Ref       | Format     |
|-----------|------------|
| 4-5090174 | 5 x 1.0 mL |



### TECHNOVIEW® Rivaroxaban Cont Low



| Ref       | Format     |
|-----------|------------|
| 4-5090172 | 5 x 1.0 mL |



### TECHNOVIEW® Rivaroxaban Cont Medium



| Ref       | Format     |
|-----------|------------|
| 4-5090173 | 5 x 1.0 mL |



## DOAC NEUTRALIZATION

### DOAC-Stop Liquid™



| Ref          | Format     |
|--------------|------------|
| 20-X9905-100 | 1 x 2.0 mL |



### DOAC-Stop™



| Ref           | Format  |
|---------------|---------|
| 20-HX9904-100 | 1 x 100 |
| 20-HX9904-50  | 1 x 50  |



# ANTICOAGULANT MONITORING

## APIXABAN

### TECHNOVIEW® Apixaban Cal Set

| Ref       | Format     |
|-----------|------------|
| 4-5090269 | 5 x 1.0 mL |



### TECHNOVIEW® Apixaban Cont High

| Ref       | Format     |
|-----------|------------|
| 4-5090270 | 5 x 1.0 mL |



### TECHNOVIEW® Apixaban Cont Low

| Ref       | Format     |
|-----------|------------|
| 4-5090271 | 5 x 1.0 mL |



## EXPLANATION FOR SYMBOLS USED



These kits are manufactured in accordance with the 98/79 EC directive for in vitro diagnostic devices. Only CE marked products can be used for diagnostic applications in Europe.



These kits are intended for in vitro diagnostic use.



These kits are for research use only and are not intended to be used for diagnostic procedures.

**FDA**

Federal Drug Administration, FDA validates diagnostic kits for in vitro diagnostic use in the United States.



Biological risk products



Storage between 2 and 8 ° C



Reactive in liquid form



Reactive in lyophilized form



Reactive in frozen form



Stability after opening at 2-8 ° C



Products that can be refrozen



Stability 12 months after refreezing at -20 ° C



Manufacturer



Importer



Distributor

# Your order

1

## To order, several possibilities

|              |  |
|--------------|--|
| By telephone | +33(0)4 67 10 71 20                                      |
| By fax       | +33(0)4 67 10 71 21                                      |
| By e-mail    | contact@cryopep.com                                      |
| By letter    | CRYOPEP, 83 rue Yves Montand, 34 080 Montpellier, FRANCE |

2

## Command Processing

We carefully pack frozen products in boxes with dry ice or cold packs according of the nature of the product.

To optimize the conditions of transport of our products, we ship our packages in dry ice only from Monday to Wednesday, except urgent customer requests.

All other orders for freeze-dried products are shipped from Monday to Friday.

3

## Transport

We work exclusively with carriers receiving ISO 9001 and CERTIPHARM certifications.

We guarantee timely delivery of all products.

During transportation, we follow all our shipments and, if necessary, call our customers to check that the packages have been received in the laboratory.

Visit our website : <https://www.cryopep.com>