


Cryopep



Cryogenics at the service of haemostasis

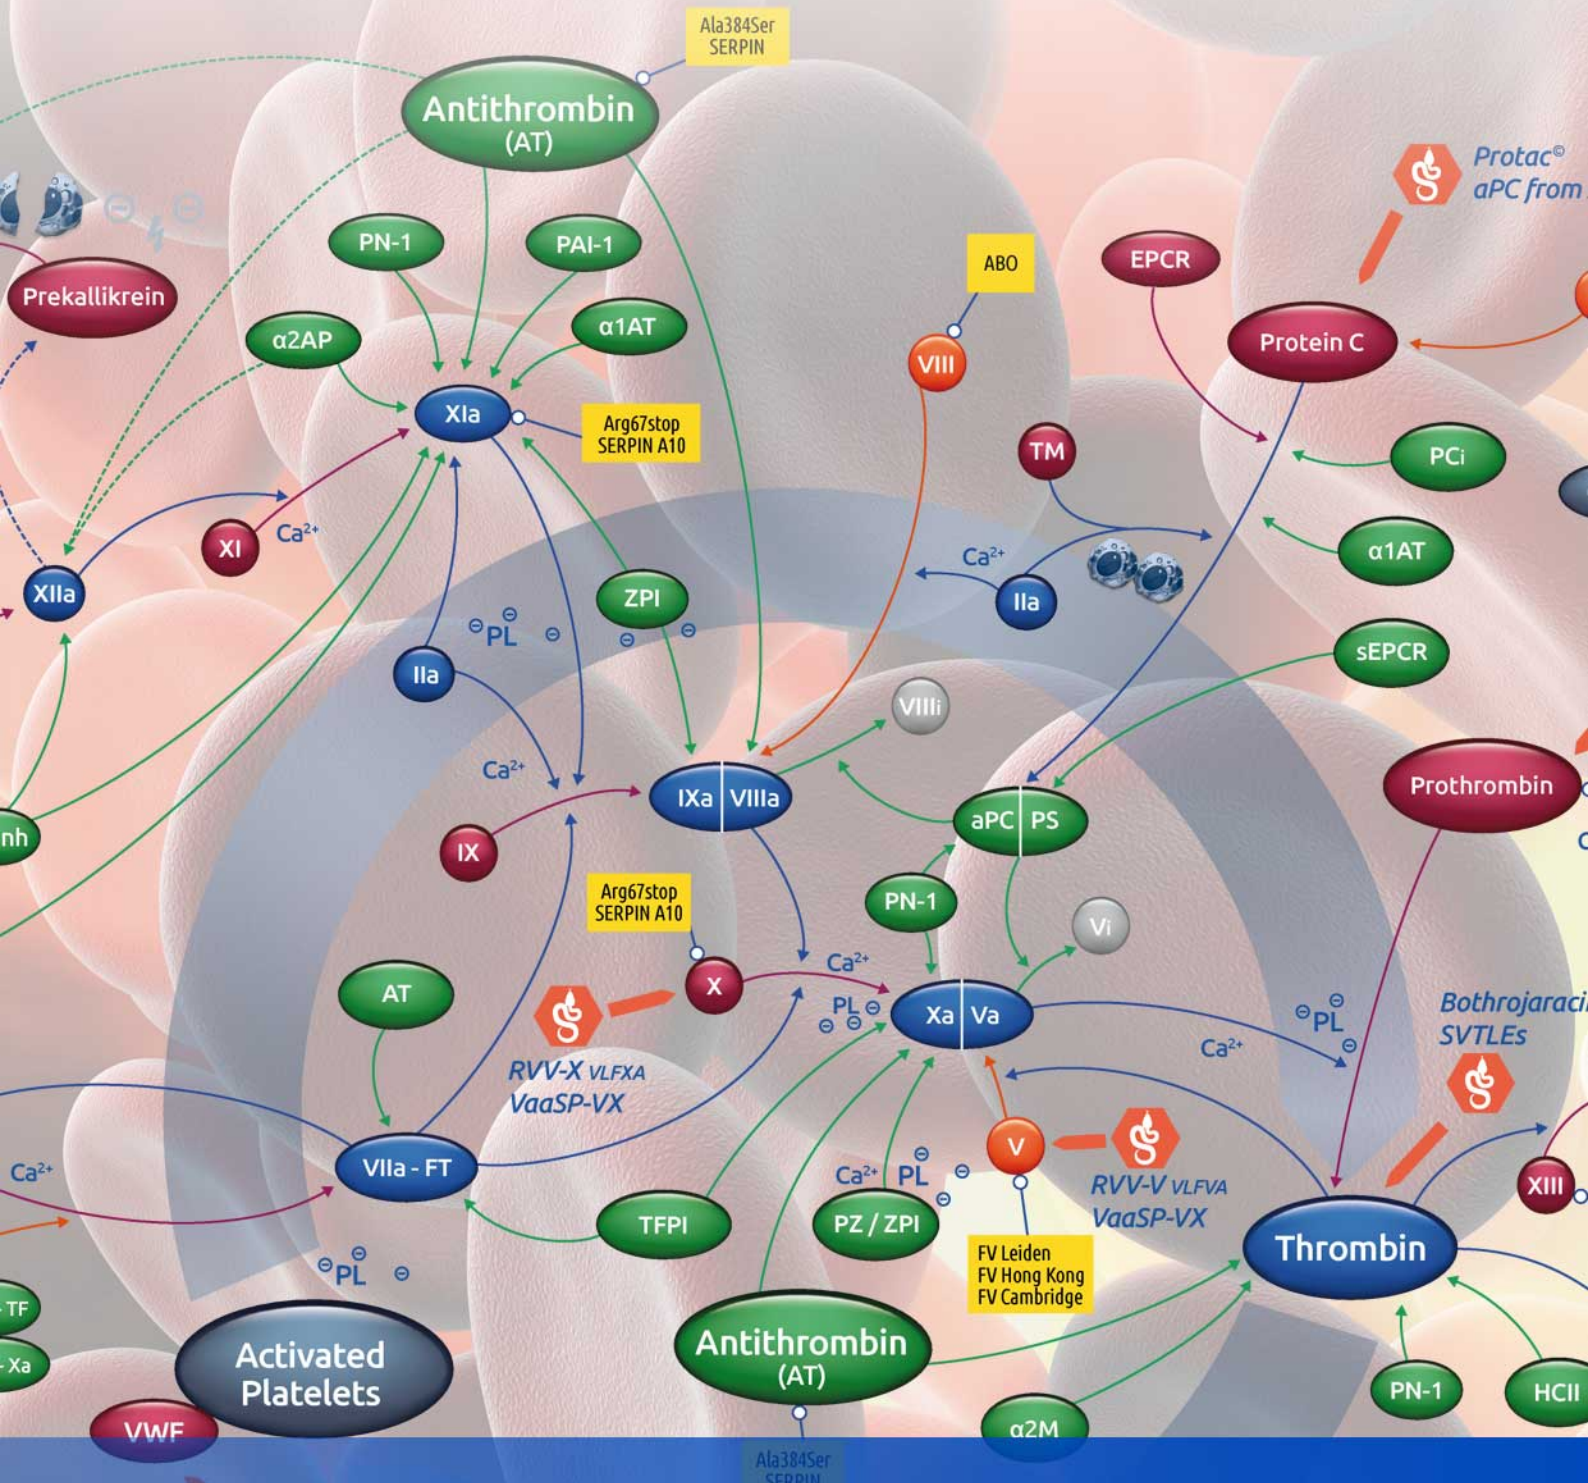

FIBRINOLYSIS

Edition of 2024-04-11 14:04:00

Botrocetin
Bitiscetin
Kaouthiagin

Endothelial Cells

Bilnexin
Convulxin
Echicetin
EMS16

Mucetin
Rhodocytin
Sochicetin-A
Triwaglerin

way

FIBRONECTIN, VITRONECTIN

TECHNOZYM® FIBRONECTIN ELISA Kit

Ref	Format
4-TC12030	12 x 8 assays



TECHNOZYM® VITRONECTIN ELISA Kit

Ref	Format
4-TC12120	12 x 8 assays



GLU-PLASMINOGEN, D-DIMERS

TECHNOZYM® D-DIMER ELISA Kit

Ref	Format
4-2599006	12 x 8 assays



TECHNOZYM® Glu-Plasminogen ELISA Kit

Ref	Format
4-TC12040	12 x 8 assays



TISSUE PLASMINOGEN ACTIVATOR

ANTIGEN

TECHNOZYM® t-PA Ag EDTA ELISA

Ref	Format
4-TC12007	12 x 8 assays



TECHNOZYM® t-PA Calibrator Set

Ref	Format
4-TC12001	5 x 0.5 mL



TECHNOZYM® t-PA Control Set

Ref	Format
4-TC12003	2 x 0.5 mL



t-PA ANTIGEN

TECHNOZYM® t-PA Combi Actibind® ELISA Kit

Ref	Format
4-TC16000	12 x 8 assays



t-PA – PAI-1 COMPLEX

TECHNOZYM® t-PA-PAI-1 Complex ELISA

Ref	Format
4-TC12080	12 x 8 assays



FIBRINOLYSIS

UROKINASE PLASMINOGEN ACTIVATOR

TECHNOZYM® u-PA Combi Actibind® ELISA Kit

Ref	Format
4-TC16010	12 x 8 assays



TECHNOZYM® u-PA ELISA Kit

Ref	Format
4-TC12010	12 x 8 assays



PLASMIN ANTIPLASMIN COMPLEX

TECHNOZYM® PAP Calibrator Set

Ref	Format
4-TC12062	5 x 0.5 mL



TECHNOZYM® PAP Complex ELISA Kit

Ref	Format
4-TC12060	12 x 8 assays



TECHNOZYM® PAP Control Set

Ref	Format
4-TC12064	2 x 0.5 mL



PLASMINOGEN ACTIVATOR INHIBITOR

IMUBIND® Tissue PAI-1 ELISA

Ref	Format
11-821	96 assays



TECHNOZYM® PAI-1 Actibind® Calibrator Set

Ref	Format
4-TC16077	5 x 0.2 mL



TECHNOZYM® PAI-1 Actibind® Control Set

Ref	Format
4-TC16079	2 x 0.2 mL



TECHNOZYM® PAI-1 Actibind® ELISA Kit

Ref	Format
4-TC16075	12 x 8 assays



TECHNOZYM® PAI-1 Antigen Calibrator Set

Ref	Format
4-TC12077	5 x 0.5 mL



TECHNOZYM® PAI-1 Antigen Control Set

Ref	Format
4-TC12079	2 x 0.5 mL



TECHNOZYM® PAI-1 Antigen ELISA Kit

Ref	Format
4-TC12075	12 x 8 assays



EXPLANATION FOR SYMBOLS USED



These kits are manufactured in accordance with the 98/79 EC directive for in vitro diagnostic devices. Only CE marked products can be used for diagnostic applications in Europe.



These kits are intended for in vitro diagnostic use.



These kits are for research use only and are not intended to be used for diagnostic procedures.



Federal Drug Administration, FDA validates diagnostic kits for in vitro diagnostic use in the United States.



Biological risk products



Storage between 2 and 8 ° C



Reactive in liquid form



Reactive in lyophilized form



Reactive in frozen form



Stability after opening at 2-8 ° C



Products that can be refrozen



Stability 12 months after refreezing at -20 ° C



Manufacturer



Importer



Distributor

Your order

1

To order, several possibilities

By telephone	+33(0)4 67 10 71 20
By fax	+33(0)4 67 10 71 21
By e-mail	contact@cryopep.com
By letter	CRYOPEP, 83 rue Yves Montand, 34 080 Montpellier, FRANCE

2

Command Processing

We carefully pack frozen products in boxes with dry ice or cold packs according of the nature of the product.

To optimize the conditions of transport of our products, we ship our packages in dry ice only from Monday to Wednesday, except urgent customer requests.

All other orders for freeze-dried products are shipped from Monday to Friday.

3

Transport

We work exclusively with carriers receiving ISO 9001 and CERTIPHARM certifications.

We guarantee timely delivery of all products.

During transportation, we follow all our shipments and, if necessary, call our customers to check that the packages have been received in the laboratory.

Visit our website : <https://www.cryopep.com>